


Variation "Status" Parameter

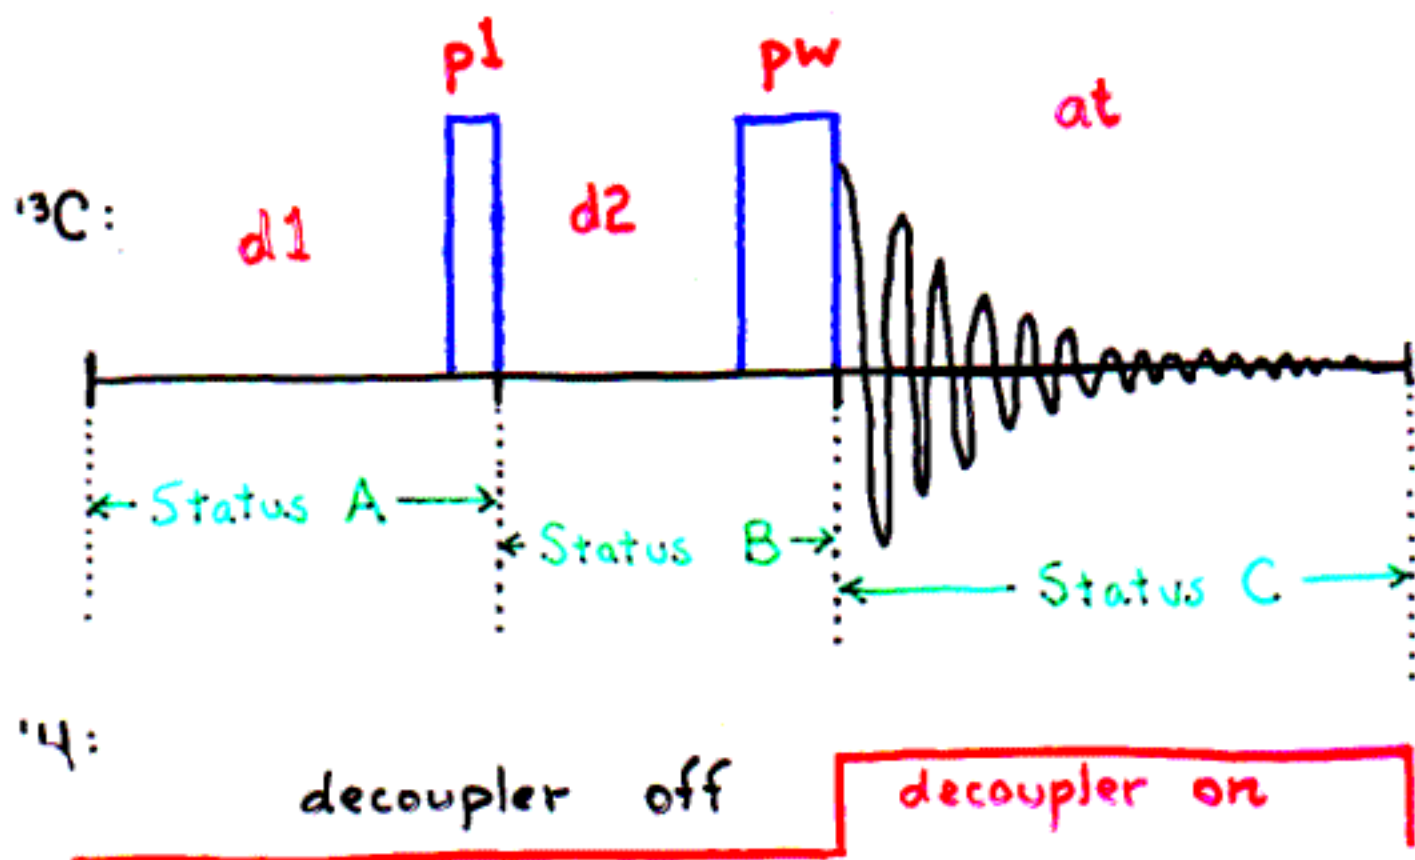

Pulse Sequence: s2pul

dm = 'nny'

decoupler mode

A B C